



BSI Standards Publication

Ophthalmic optics — Contact lenses — Hygienic management of multipatient use trial contact lenses

National foreword

This British Standard is the UK implementation of ISO 19979:2018. It supersedes [PD ISO/TS 19979:2014](#), which is withdrawn.

The UK participation in its preparation was entrusted to Technical Committee CH/172/9, Contact lenses and contact lens care products.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© The British Standards Institution 2018
Published by BSI Standards Limited 2018

ISBN 978 0 580 90884 2

ICS 11.040.70

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 March 2018.

Amendments/corrigenda issued since publication

Date	Text affected
------	---------------

INTERNATIONAL STANDARD

ISO
19979

First edition
2018-03-15

Ophthalmic optics — Contact lenses — Hygienic management of multipatient use trial contact lenses

*Optique ophtalmique — Lentilles de contact — Entretien de l'hygiène
des lentilles de contact d'essai à usage multipatient*



Reference number
ISO 19979:2018(E)

© ISO 2018



COPYRIGHT PROTECTED DOCUMENT

© ISO 2018, Published in Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Ch. de Blandonnet 8 • CP 401
CH-1214 Vernier, Geneva,
Switzerland
Tel. +41 22 749 01 11 Fax
+41 22 749 09 47
copyright@iso.org
www.iso.org

Contents

Page

Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Methods of hygienic management for multipatient use trial contact lenses	2
5 Options for hygienic management of multipatient use trial contact lenses	2
5.1 General.....	2
5.2 Disinfection procedure with moist heat.....	4
5.3 Disinfection procedures using an 3 % ophthalmic hydrogen peroxide for 3 h or equivalent.....	5
5.4 Storage of disinfected lenses.....	5
6 Flowchart to describe the use of multipatient use trial contact lenses	5
Annex A (informative) Disinfection procedure using an 3 % ophthalmic hydrogen peroxide solution	7
Bibliography	8

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see the following URL: www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 172, *Optics and photonics*, Subcommittee SC 7, *Ophthalmic optics and instruments*.

This first edition of ISO 19979:2018 cancels and replaces ISO/TS 19979:2014, which has been technically revised. In addition to the change in document type from a Technical Specification to an International Standard, the main changes compared to ISO/TS 19979:2014 are as follows:

- the specific processes of hygienic management have been presented as tables;
- a flow chart of the hygienic management process has been introduced;
- the example of disinfection procedure using hydrogen peroxide has been moved to [Annex A](#);
- editorial revisions have been implemented.

Introduction

Wherever possible, a trial contact lens should be used only on one individual. While the current trend in contact lens development is toward disposable and extended wear lenses, conventional lenses including rigid gas-permeable (RGP) contact lenses, composite contact lenses and hydrogel contact lenses in special designs and parameters are necessary to meet individual patient needs.

The reconditioning of multipatient use contact lenses involves cleaning, disinfection and storage of the contact lenses. The cleaning step is not specified in this document, as it does not differ from the cleaning of contact lenses for end-users.

The hygienic management for multipatient use differs from the requirements of hygienic management for contact lenses for individual use and from surface disinfection used in hospitals.

This document gives guidance for the development of instructions for manufacturers of multipatient use contact lenses, in order to mitigate the risk of pathogen transfer between patients.

Ophthalmic optics — Contact lenses — Hygienic management of multipatient use trial contact lenses

1 Scope

This document provides guidance to manufacturers for the development of information to be provided to eye care practitioners for the hygienic management of trial hydrogel, composite and rigid gas-permeable (RGP) contact lenses intended for multipatient use.

This document does not apply to:

- labelling of contact lenses;
- the inactivation of prions and viruses since there are no standardised methods available for contact lenses.

This document can be used as guidance for the development of a hygienic management procedure for multipatient use.

NOTE [ISO 14729](#) does not cover multipatient use.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

[ISO 18369-1](#), *Ophthalmic optics — Contact lenses — Part 1: Vocabulary, classification system and recommendations for labelling specifications*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in [ISO 18369-1](#) and the following apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- IEC Electropedia: available at <http://www.electropedia.org/>
- ISO Online browsing platform: available at <https://www.iso.org/obp>

3.1

trial contact lens

diagnostic contact lens

contact lens only used by a practitioner or fitter for the purpose of selecting the appropriate contact lens parameters for the intended wearer

[SOURCE: ISO 18369-1:2017, 3.1.10.8]

3.2

multipatient use trial contact lens

trial contact lens permitted to be used on more than one person

[SOURCE: ISO 18369-1:2017, 3.1.10.9, modified — Note 1 to entry has been deleted.]

3.3 competent personnel

personnel, qualified or trained for the hygienic conditioning of contact lenses

3.4 composite contact lens

contact lens composed of two or more different materials

[SOURCE: ISO 18369-1:2017, 3.1.1.11, modified — The example has been deleted.]

4 Methods of hygienic management for multipatient use trial contact lenses

The ideal approach for trial contact lenses is to use the lens a single time, after which the lens is dispensed to the same individual or discarded. Where reuse is necessary, moist heat management is preferred over chemical management whenever applicable.

The manufacturer shall provide instructions for the hygienic management of multipatient use trial contact lenses appropriate to the type of lens being used.

The instructions shall include advice on the process to be applied and on how to maintain the processed contact lens in a suitable condition (e.g. container choice, container closure).

Ocular irritation due to use of a chemical disinfection method should be considered.

When using this document as guidance for the development of a hygienic management procedure for multipatient use, the disinfection performance shall be appropriate to meet at least the requirements in [Clause 5](#).

5 Options for hygienic management of multipatient use trial contact lenses

5.1 General

[Table 1](#) gives general information on relevant items for the hygienic management of multipatient use trial contact lenses.

Table 1 — General information

	Content	Action	NOTE
1	Precautions against infections	Dispose of contact lenses used in persons known to be infected with <ul style="list-style-type: none"> — Herpes simplex cornea; — Hepatitis; — Human Immunodeficiency Virus (HIV); — Adenovirus. 	Use disposable/single use gloves. Dispose of trial contact lenses immediately after use. There is a possibility that National Regulations add other infectious diseases to this list. Practitioners should be instructed to monitor Health Authority communications for emerging risks related to outbreaks of unknown or little known infectious diseases, and associated advice.

	Content	Action	NOTE
2	Waste disposal	When it is necessary to dispose of any lenses, containers, or solutions due to reasons mentioned in 1, the items need to be treated as “biohazardous” waste. Use disposable/single use powder-free, latex-free gloves to remove the infected lenses from patient eyes. If necessary, dispose of containers and solutions used in contact with the infected lenses. The lenses, containers and solutions shall be treated as “biohazardous waste”.	The local requirements for the disposal of biohazardous waste apply.
3	Workbench surface	Shall be cleaned and disinfected on a daily basis with a suitable surface disinfectant.	
4	Hand washing	Wash your hands before and after each patient fitting with a surgical scrub or a liquid soap. Dry your hands on a new paper towel.	Drying the hands reduces the chances of spreading water-borne organisms such as <i>Acanthamoeba</i> .
a)		Hand washing is required even before the use of gloves.	Information on hygienic hand wash is provided on the poster by WHO: www.who.int/gpsc/5may/How_To_HandWash_Poster.pdf .
5	Cleaning of contact lenses	Rub and rinse the contact lens before (RGP only) and after use according to the instructions of the manufacturer.	Removing particulate debris from a contact lens ensures a more effective use of the disinfecting solution.
6	Applicable procedures	The manufacturer shall specify the methods of disinfection (e.g. moist heat disinfection or an ophthalmic hydrogen peroxide treatment) to be used during hygienic management.	Moist heat disinfection is applicable for hydrogel lenses. (See Table 2). Most contact lens types can be disinfected using an ophthalmic hydrogen peroxide solution.
7	Number of re-uses or time in use	All lenses stored in a soaking solution or in a dry condition shall be discarded after X times of use or after Y months from first use, or if the lens is damaged, whichever comes first.	For lenses stored in soaking solution, repeat the disinfection procedures if the contact lens has not been used for 28 d. The lens manufacturer shall determine the numbers X and Y. If the manufacturer is aware of particular changes/damages that may occur, the manufacturer shall provide guidance on related criteria for discarding the lens.
8	Re-use of contact lenses	The contact lens shall be inspected before and after every use. If the lens is damaged or its physical appearance has changed, the lens shall be discarded.	

	Content	Action	NOTE
9	Contact lens container	The manufacturer shall state the type of container suitable for the hygienic management of multipatient use trial contact lenses. The methods shall be stated by which the container can be cleaned, properly closed, and relabelled, if appropriate.	
a)		Information on regular replacement and care of the containers shall be given by the contact lens manufacturer.	
10	Documentation	The manufacturer shall specify: <ul style="list-style-type: none"> — lot number; — lens parameters; — expiry date; — if appropriate maximum number of uses. 	Enough lens parameters should be given to sufficiently identify the lens and enable traceability.
11	Record of each disinfection procedure	Type of procedure, e.g. chemical management, moist heat disinfection.	
a)		Practitioners shall record: <ul style="list-style-type: none"> — patient's reference; — date of use; — date of hygienic management; — contact lens details. 	
b)		Person performing disinfection	Competent personnel only, with supporting training records.
12	Storage container labelling	<ul style="list-style-type: none"> — parameters of contained contact lens; — lot number; — date of disinfection; — lens identification (for future tracking). 	Add sufficient information to identify individual lens.

5.2 Disinfection procedure with moist heat

[Table 2](#) gives guidance on factors to be considered for disinfection with moist heat.

NOTE Only after a properly validated sterilization process, according to [ISO/TS 17665-2:2009](#), Table 1, can the lens be described as sterile.

Table 2 — Disinfection procedure with moist heat (applicable for hydrogel lenses only)

	Procedure step	Example
Preparation	Choice of medium, in which to place the lens.	Saline (0,9 % sodium chloride solution).
	Choice of container.	Borosilicate glass vial with crimped seal.

	Procedure step	Example
Procedure	Choice of disinfection process conditions.	Target temperature 134 °C for dwell time of at least 3 min, or Target temperature 121 °C for dwell time of at least 15 min.

5.3 Disinfection procedures using an 3 % ophthalmic hydrogen peroxide for 3 h or equivalent

The recommended disinfection solution shall have intrinsic disinfecting efficacy equivalent to a 3 h exposure to 3 % ophthalmic hydrogen peroxide. Equivalence may be demonstrated empirically.

NOTE An example of a disinfection procedure using hydrogen peroxide is provided in [Annex A](#).

5.4 Storage of disinfected lenses

[Table 3](#) gives additional information on the storage of disinfected lenses.

Table 3 — Storage of disinfected lenses

	Step	Procedure	Information
1	Preparation for storage	Fill appropriate container with stipulated preserved soaking solution.	Hydrogel contact lenses should not be stored dry.
a)		To avoid skin contact, use disinfected tweezers.	This is not appropriate for moist heat processed lenses.
b)		Re-insert lens/holder and close the container.	Container of moist heat processed lenses shall not be opened until use.
2	Duration of storage	The contact lens manufacturer shall state the maximum number of times of re-use and the maximum duration of time from the first use as a multipatient use trial contact lens.	Applicable for hydrogel, composite, and RGP lenses.
3	Wet storage	The validation of the system used defines the storage time.	Applicable for hydrogel, composite, and RGP lenses.
4	Dry storage	Dry contact lens with a clean lint-free paper tissue.	Applicable for RGP lenses only.
a)		Insert lens in an appropriate container and close securely. A dry stored lens should be prepared for reuse.	

6 Flowchart to describe the use of multipatient use trial contact lenses

See [Figure 1](#).

Disinfection procedure applicable for RGP lenses, hydrogel and composite lenses.

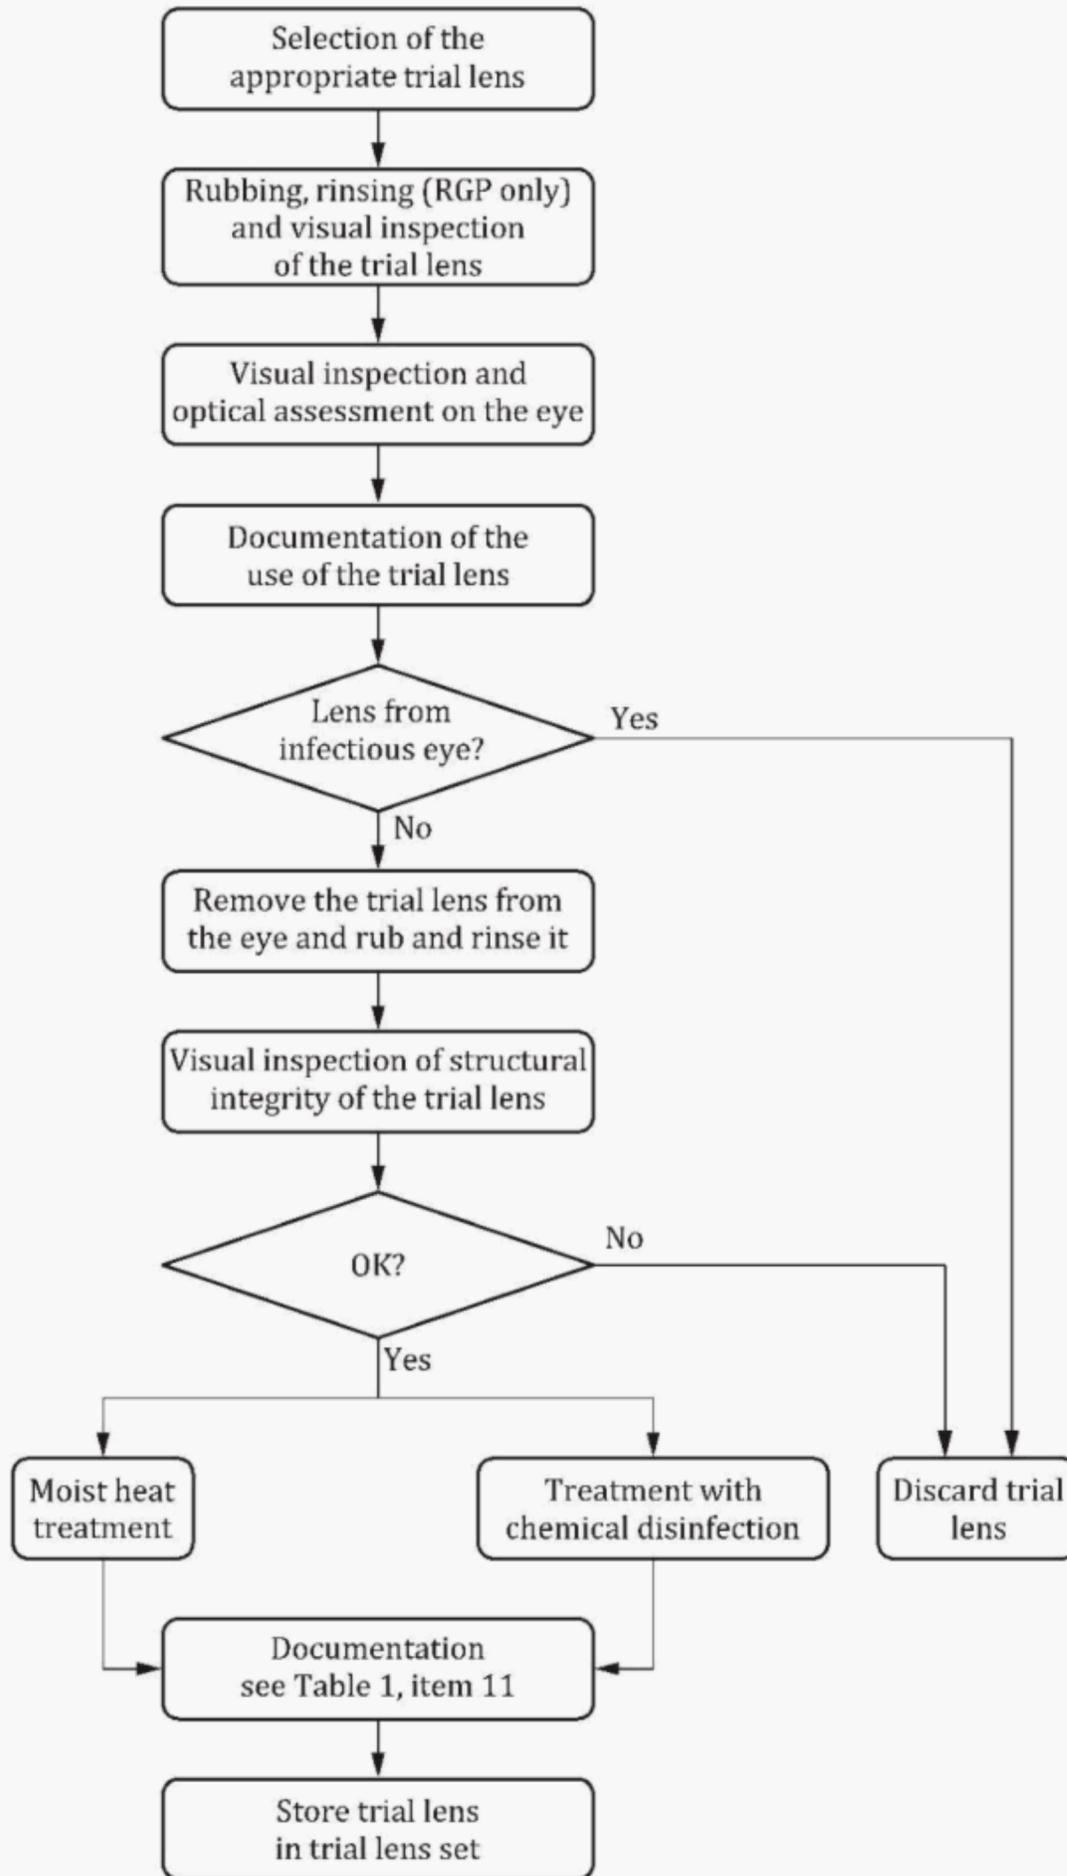


Figure 1 — Use of multipatient use trial contact lenses

Annex A (informative)

Disinfection procedure using an 3 % ophthalmic hydrogen peroxide solution

[Table A.1](#) provides additional information on the disinfection procedure with an ophthalmic hydrogen peroxide solution.

Table A.1 — Disinfection procedure using an 3 % ophthalmic hydrogen peroxide (H₂O₂)-solution (applicable for RGP, composite and hydrogel lenses)

	Step	Procedure	Information
1	Preparation	Use the contact lens case and/or holder recommended by the manufacturer.	It is possible to apply products for end-user, but the requirements of multipatient-use shall be fulfilled.
2	Procedure	Fill container with 3 % ophthalmic hydrogen peroxide solution.	
a)		Close the lens container securely.	
3	Disinfection	Soak the lens according to the information provided by the manufacturer for at least 3 h, prior to the recommended neutralization procedure.	One step hydrogen peroxide systems are not appropriate.
4	Neutralization	Add neutralization tablet or discard peroxide solution and refill container with appropriate volume of neutralization solution. Securely tighten the cap.	The manufacturer of the neutralizing product defines the neutralization time.
a)		Shake vigorously for 10 s to 15 s and soak for the appropriate neutralization time.	
b)		Open lens case, remove lens holder. Shake off residual drops. Discard the neutralizing solution.	

Bibliography

- [1] [ISO 11981](#), *Ophthalmic optics — Contact lenses and contact lens care products — Determination of physical compatibility of contact lens care products with contact lenses*
- [2] [ISO 11987](#), *Ophthalmic optics — Contact lenses — Determination of shelf-life*
- [3] ISO/TS 11139, *Sterilization of health care products — Vocabulary*
- [4] [ISO 14729](#), *Ophthalmic optics — Contact lens care products — Microbiological requirements and test methods for products and regimens for hygienic management of contact lenses*
- [5] [ISO 17664](#), *Processing of health care products — Information to be provided by the medical device manufacturer for the processing of medical devices*
- [6] [ISO 17665-1](#), *Sterilization of health care products — Moist heat — Part 1: Requirements for the development, validation and routine control of a sterilization process for medical devices*
- [7] [ISO/TS 17665-2](#), *Sterilization of health care products — Moist heat — Part 2: Guidance on the application of ISO 17665-1*
- [8] Centers for Disease Control. Recommendations for preventing possible transmission of human T-lymphotropic virus type III/lymphadenopathy-associated virus from tears. *Morbidity and Mortality Weekly Report*. 1985, **34** pp. 533–534
- [9] Lichter P. Controlling risks of the possible transmission of human immunodeficiency virus. *Ophthalmology*. 1989, **96** p. 1
- [10] Smith C.A., & Pepose J.S. Disinfection of tonometers and contact lenses in the office setting: are current techniques adequate? *Am. J. Ophthalmol.* 1999, **127** pp. 77–84
- [11] Anger C., Ambrus K., Stoecker J., Kapadia S., Thomas L. Antimicrobial Efficacy of Hydrogen Peroxide for Contact Lens Disinfection. *Contact Lens Spectrum*. 1990, **5** pp. 46–51
- [12] Lakkis C., Lian K.-Y., Napper G., Kiel y P.M. Infection control guidelines for optometrists 2007. *Clin. Exp. Optom.* 2007, **90** (6) pp. 434–444

British Standards Institution (BSI)

BSI is the national body responsible for preparing British Standards and other standards-related publications, information and services.

BSI is incorporated by Royal Charter. British Standards and other standardization products are published by BSI Standards Limited.

About us

We bring together business, industry, government, consumers, innovators and others to shape their combined experience and expertise into standards-based solutions.

The knowledge embodied in our standards has been carefully assembled in a dependable format and refined through our open consultation process. Organizations of all sizes and across all sectors choose standards to help them achieve their goals.

Information on standards

We can provide you with the knowledge that your organization needs to succeed. Find out more about British Standards by visiting our website at bsigroup.com/standards or contacting our Customer Services team or Knowledge Centre.

Buying standards

You can buy and download PDF versions of BSI publications, including British and adopted European and international standards, through our website at bsigroup.com/shop, where hard copies can also be purchased.

If you need international and foreign standards from other Standards Development Organizations, hard copies can be ordered from our Customer Services team.

Copyright in BSI publications

All the content in BSI publications, including British Standards, is the property of and copyrighted by BSI or some person or entity that owns copyright in the information used (such as the international standardization bodies) and has formally licensed such information to BSI for commercial publication and use.

Save for the provisions below, you may not transfer, share or disseminate any portion of the standard to any other person. You may not adapt, distribute, commercially exploit, or publicly display the standard or any portion thereof in any manner whatsoever without BSI's prior written consent.

Storing and using standards

Standards purchased in soft copy format:

- A British Standard purchased in soft copy format is licensed to a sole named user for personal or internal company use only.
- The standard may be stored on more than 1 device provided that it is accessible by the sole named user only and that only 1 copy is accessed at any one time.
- A single paper copy may be printed for personal or internal company use only.
- Standards purchased in hard copy format:
- A British Standard purchased in hard copy format is for personal or internal company use only.
- It may not be further reproduced – in any format – to create an additional copy. This includes scanning of the document.

If you need more than 1 copy of the document, or if you wish to share the document on an internal network, you can save money by choosing a subscription product (see 'Subscriptions').

Reproducing extracts

For permission to reproduce content from BSI publications contact the BSI Copyright & Licensing team.

Subscriptions

Our range of subscription services are designed to make using standards easier for you. For further information on our subscription products go to bsigroup.com/subscriptions. With British Standards Online (BSOL) you'll have instant access to over 55,000 British and adopted European and international standards from your desktop. It's available 24/7 and is refreshed daily so you'll always be up to date.

You can keep in touch with standards developments and receive substantial discounts on the purchase price of standards, both in single copy and subscription format, by becoming a BSI Subscribing Member. PLUS is an updating service exclusive to BSI Subscribing Members. You will automatically receive the latest hard copy of your standards when they're revised or replaced.

To find out more about becoming a BSI Subscribing Member and the benefits of membership, please visit bsigroup.com/shop.

With a Multi-User Network Licence (MUNL) you are able to host standards publications on your intranet. Licences can cover as few or as many users as you wish. With updates supplied as soon as they're available, you can be sure your documentation is current. For further information, email subscriptions@bsigroup.com.

Revisions

Our British Standards and other publications are updated by amendment or revision. We continually improve the quality of our products and services to benefit your business. If you find an inaccuracy or ambiguity within a British Standard or other BSI publication please inform the Knowledge Centre.

Useful Contacts

Customer Services
Tel: +44 345 086 9001
Email (orders): orders@bsigroup.com
Email (enquiries): cservices@bsigroup.com

Subscriptions
Tel: +44 345 086 9001
Email: subscriptions@bsigroup.com

Knowledge Centre
Tel: +44 20 8996 7004
Email:
knowledgecentre@bsigroup.com

Copyright & Licensing
Tel: +44 20 8996 7070
Email: copyright@bsigroup.com

BSI Group Headquarters

389 Chiswick High Road London W4 4AL UK

This page deliberately left blank